

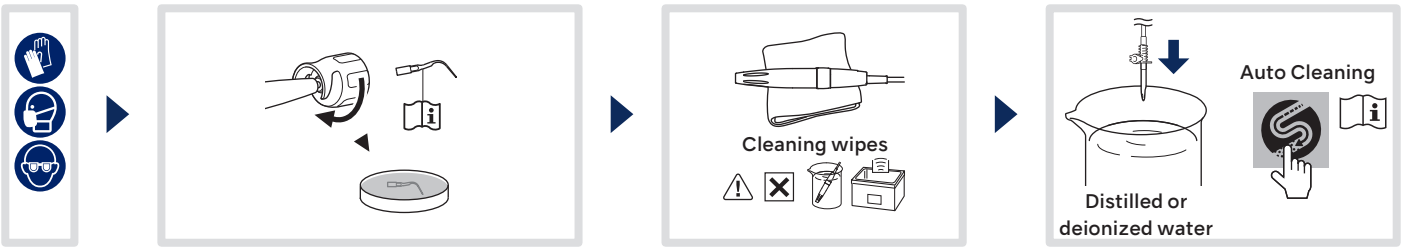


### 1 Preparation

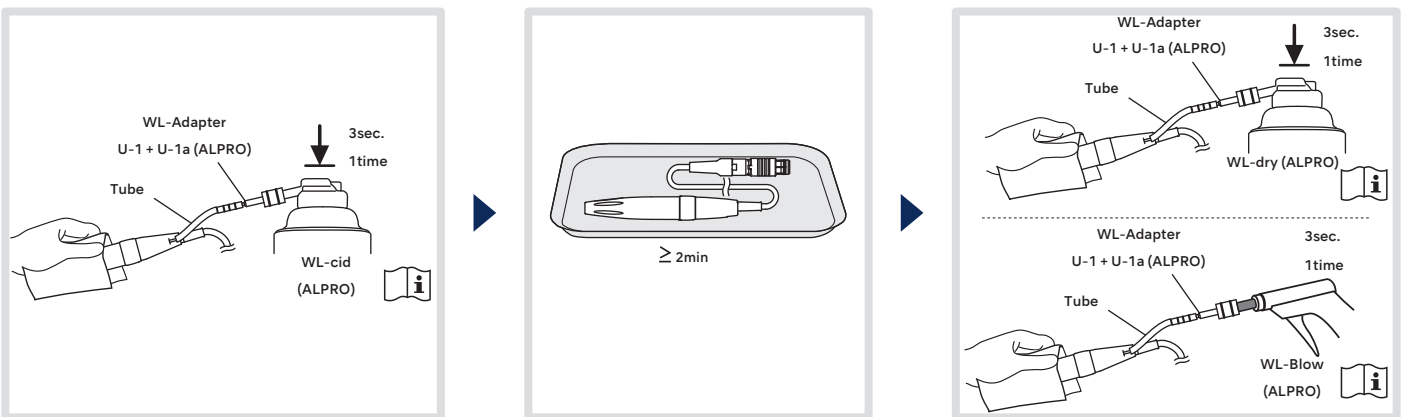


### 2 Cleaning, Disinfection and Drying

#### Manual

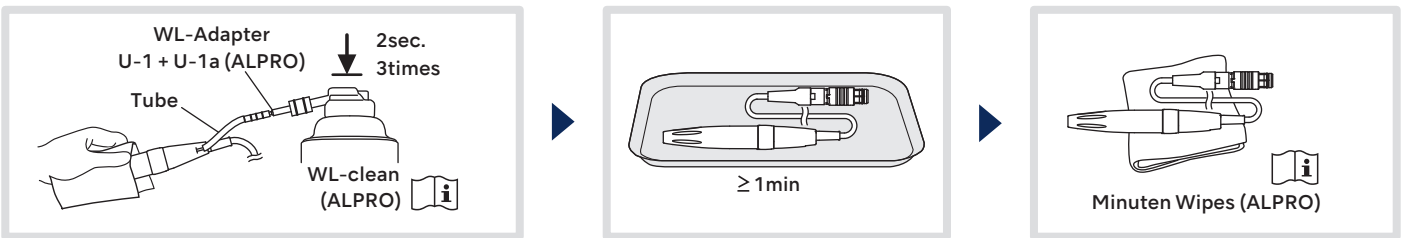


#### Automated

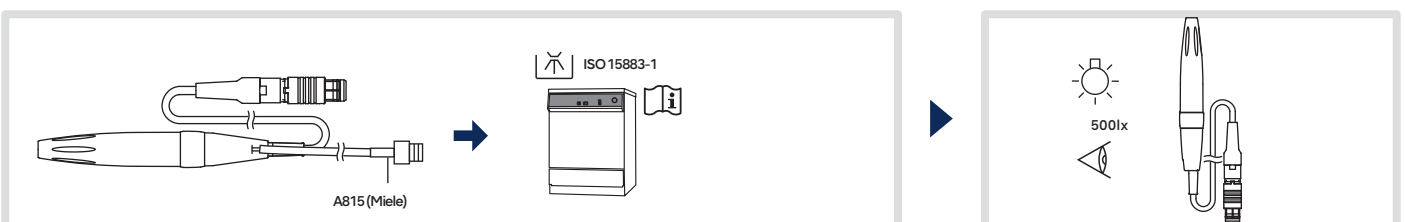





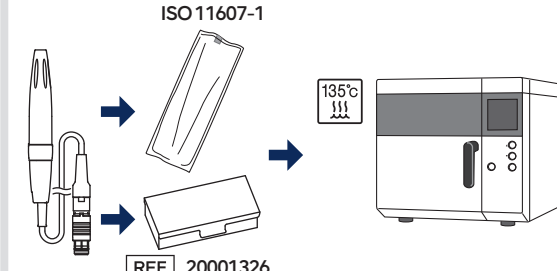

- ⚠ Cover the product with a cloth when drying with compressed air to prevent water aerosol from being produced.
- Use a nationally approved disinfectant with proven bactericidal, fungicidal, and virucidal properties.

### 3 Packaging, Sterilizing and Drying



| Type            | Class N | Class B |
|-----------------|---------|---------|
| Temperature     | 132°C   | 134°C   |
| Full Cycle Time | ≥15min  | 3-18min |
| Drying Time     | ≥30min  | ≥30min  |


  
**CAUTION**



**Steam sterilization**
  




Use a sterilization pouch that conforms to ISO 11607-1. Seal the pouch.  
 Maximum temperature for NSK instruments is 135°C.

Perform steam sterilization using the conditions above.  
 Use a steam sterilizer to perform sterilization.

### 4 Storage

